



Another Effective and Innovative Product from AMI

THE DELVE™ Pat. Pend.
Trocar Sleeve Cleaning Device


Blood & fluids splash on the camera body and specifically the lens during endoscopic procedures causing a blurry and foggy image. The camera has to be pulled out of the Trocar sleeve and the lens needs to be wiped clean and defogged. When reinserting it, the debris & fluid left in the Trocar sleeve and on the valve contaminate the lens again. The process must be repeated a few times wasting time and frustrating the medical staff. Current cleaning methods are regular sponges, raytecs, Q-Tips and other non-effective, time consuming and unsafe techniques.

SOLUTION:


The Delve cleans the inside of the Trocar sleeve and valve to prevent the camera lens from soiling upon reinsertion into the Trocar sleeve.

Features:

- Simple insertion of "The Delve" into the Trocar sleeve **ONCE**, followed by quick removal eliminates the fluid and debris inside the Trocar sleeve and valve leaving a clean path for the camera when reinserting it into the Trocar sleeve.
- Reduces the operative time and eliminates the surgeon's frustration while provide a clear view of the surgical site.

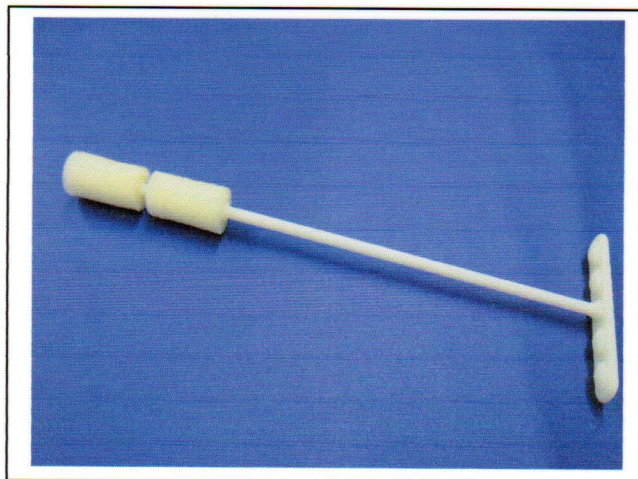

THE DELVE

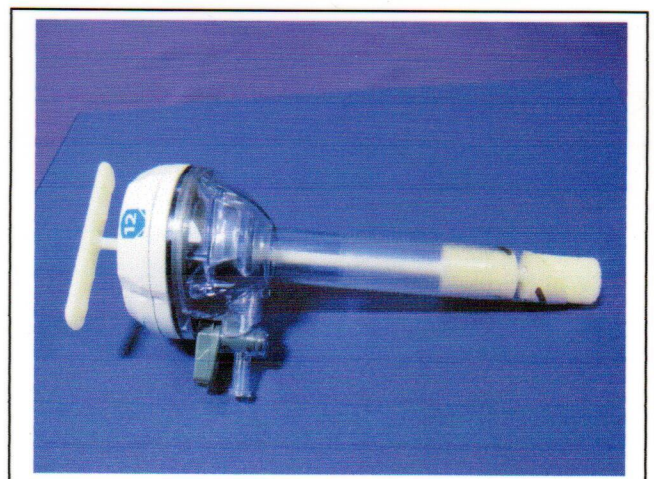

THE DELVE INSIDE A TROCAR SLEEVE

PRODUCT PART NO.	PRODUCT DESCRIPTION	PACKAGING
AM4215-5	The "Delve" 5mm Trocar cleaning device – Available 1 st Quarter, 2016	1/Ea 25/Disp 4/Disp/Case 100 Ea
AM4215-10	The "Delve" 10 - 12mm Trocar cleaning device – Available 1 st Quarter, 2016	1/Ea 25/Disp 4/Disp/Case 100 Ea
AM4215-KIT	The Dual "Delve" 5mm and 10mm with fog free and sponge – Available 1 st Quarter, 2016	1/Ea 25/Disp 2/Disp/Case 50 Ea